


Globe stereothermometer - a new instrument developed in Occupational Safety Research Institute in Prague

 25.09.2008

Kulový stereo teploměr - nový přístroj vyvinutý ve VÚBP Praha

Miloslav V. Jokl¹, Stanislav Malý³, Zdeněk Jiráček², Hana Tomášková⁴, Daniel Šebesta¹

¹ Czech Technical University, Prague, miloslav.jokl@fsv.cvut.cz

² University of Ostrava, zdenek.jirak@osu.cz

³ Occupational Safety Research Institute, Prague, malys@vubp-praha.cz

⁴ Institute of Public Health in Ostrava, hana.tomaskova@zuova.cz

kulový stereoteploměr

tepelná zátěž

sálavé teplo

komfort

Abstract

According to EN ISO 7730 the estimation of RTA ($t_{rA}-t_{rB}$) is prescribed; it has been measured by Indoor Climate Analyzer of Bruel and Kjaer. It was proved that a new instrument, globe stereothermometer, developed in Malý's research group, can be applied for this purpose. It is a globe of 15cm in diameter divided into 6 segments; the surface temperature of each segment is called stereotemperature (t_{stereo}). The mean value of all six stereotemperatures equals to globe temperature (t_g). Radiant Temperature Asymmetry can be estimated from equations (6),(7)and (8) and from Fig. 7. Stereothermometer is produced by SIPOCH Ltd. Prague. The company also developed electronics and technology of the instrument (dipl. Ing. L. Vajner). This paper introduces new method for radiant temperature asymmetry estimation.

Keywords: radiant temperature asymmetry, local comfort criteria, thermal comfort

Abstrakt

Dle EN ISO 7730 je předepsáno hodnocení RTA ($t_{rA}-t_{rB}$). Měření bylo provedeno v analytickém zařízení vnitřního klimatu. Bylo potvrzeno, že nový nástroj, tj. stereoteploměr, který byl vyvinut ve výzkumném týmu Dr. Malého, může být pro tento účel aplikován. Je to koule o průměru 15 cm, která je rozdělena do šesti segmentů; plošná teplota každého segmentu se nazývá stereoteplota (t_{stereo}). Průměrná hodnota všech šesti stereoteplot je rovná teplotě koule

(t_g). Asymetrie sálavého tepla může být vyčíslena z rovnic (6), (7) a (8) a z obrázku č. 7. Stereoteploměr je vyráběn SIPOCH, s.r.o. Praha. Tato společnost vyvíjela rovněž elektroniku a příslušnou techniku tohoto nástroje (Ing. L. Vajner). Tento příspěvek představuje novou metodu hodnocení asymetrie sálavého tepla.

Klíčová slova: sálavé teplo, tepelná zátěž, komfort, stereoteploměr

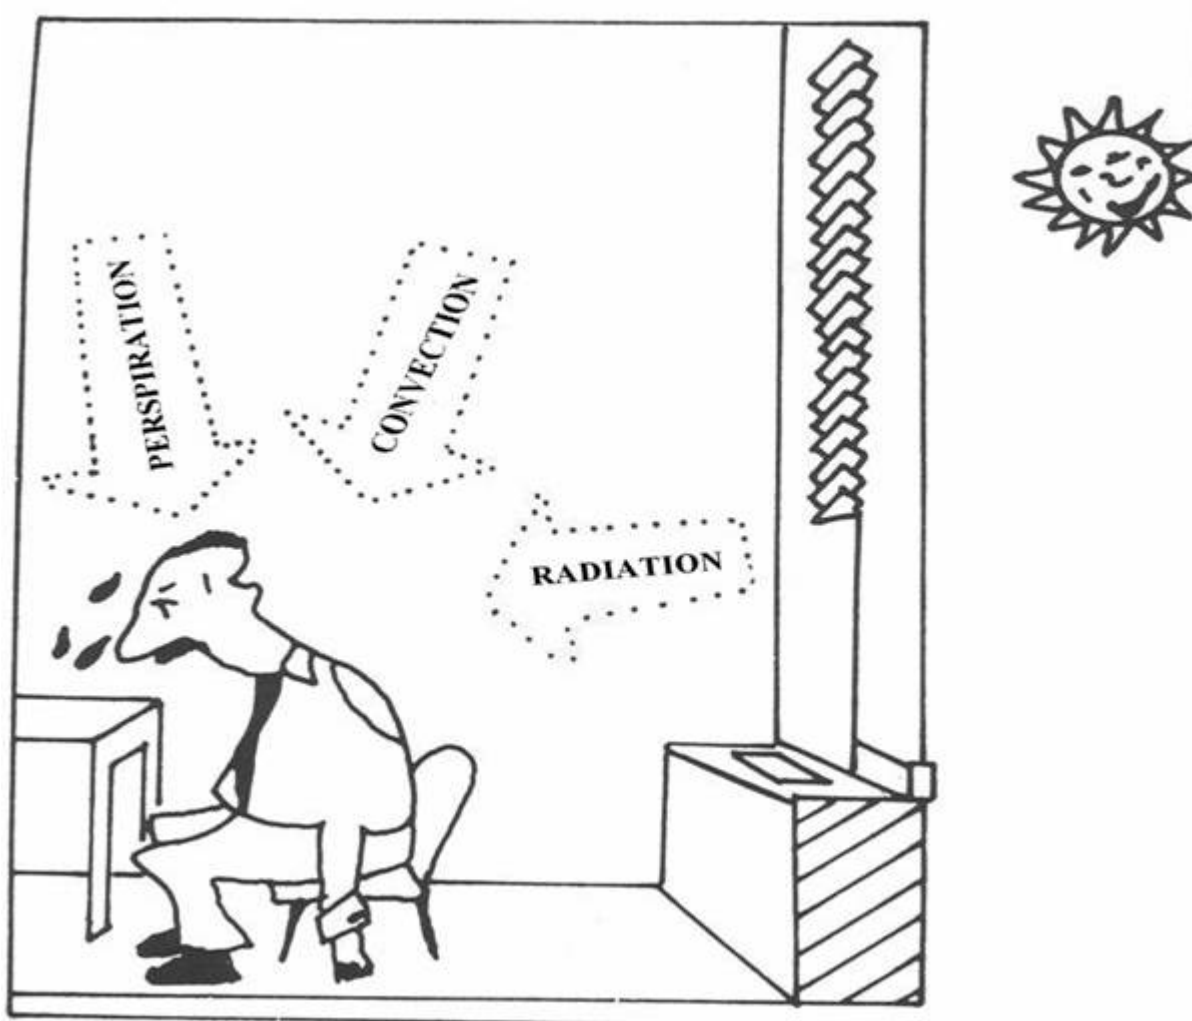


Figure 1. One side irradiation at the workplace from the window

Introduction

The so called Radiant Temperature Asymmetry (RTA) is the recommended criterion for non-uniform thermal load on human body, e.g. from radiating window (Fig. 1), heated floor, heated or cooled ceiling, the workplaces at furnaces in iron and glass works, by the standard EN ISO 7730. It is valid for three categories A, B, C depending on various predicted percentage of dissatisfied people (PPD): A is the most comfortable, for the lowest PPD, C for the highest PPD. An example of prescribed values of RTA is presented in Tab. 1 (Tab. A4 EN ISO 7730) (JOKL, 2002)(PETRÁŠ...[et al.], 2004).

Table 1. RTA by EN ISO 7730:2005

CATEGORY	RADIANT TEMPERATURE ASYMMETRY - RTA
----------	-------------------------------------

WARM CEILING	COOL WALL	COOL CEILING	WARM WALL	
A	< 5	< 10	< 14	< 23
B	< 5	< 10	< 14	< 23
C	< 7	< 13	< 18	< 35

The estimation of RTA up to now

RTA is measured up to now by Indoor Climate Analyzer type 1213, Bruel and Kjaer, Denmark. There is a special sensor for this purpose with this instrument, so called RTA (Radiant Temperature Asymmetry) transducer MM 0036 (Fig. 2), By means of PT100 radiant heat is estimated coming from two opposite sides A and B: surface temperatures t_{rA} and t_{rB} of a small plane are measured and their difference ($t_{rA} - t_{rB}$) is the RTA.

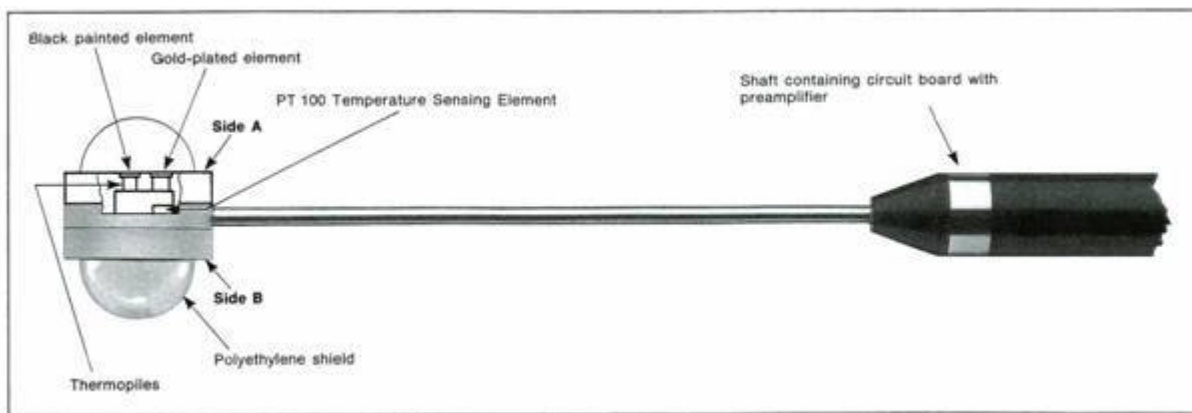


Figure 2. RTA transducer (MM 0036) of Indoor Climate Analyzer from Bruel and Kjaer

A new way of RTA estimation

It is based on a new instrument application, the so called globe stereothermometer.

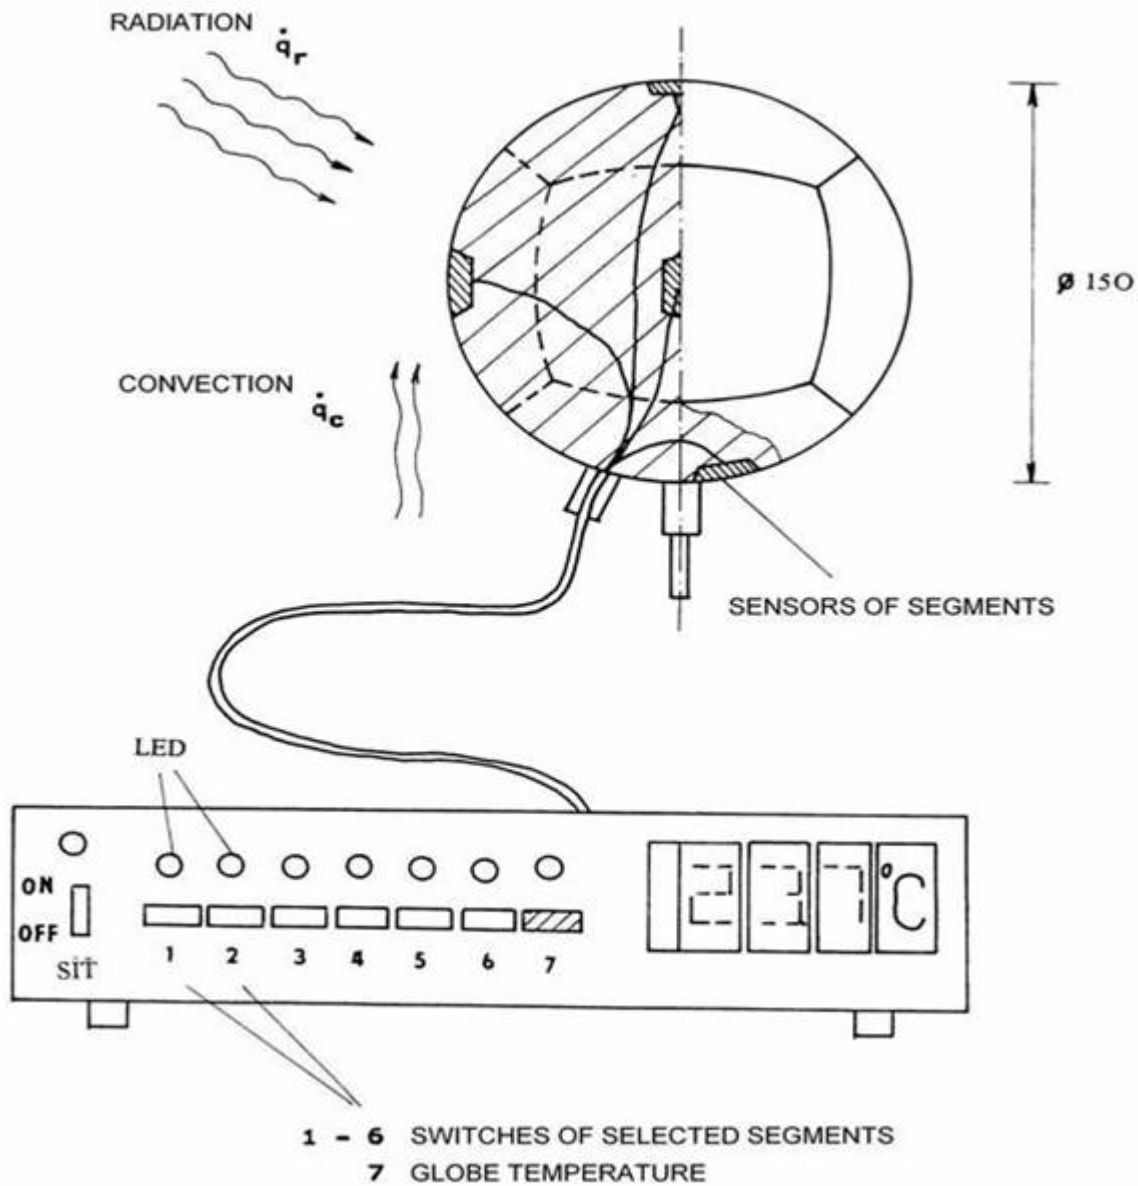


Figure 3. Globe stereothermometer scheme

Principle of stereothermometer

First have a look at an ordinary globe thermometer (GT). There is a big difference in success of GT and other instruments, developed for the same purpose: GT is used from the year 1923 continuously as a part of many national standards, government directives and hygienic prescriptions. There is a simple reason for it: - GT does not try to be a model of human body, it is only a part of human body thermal equilibrium equation, operative temperature can be substituted by globe temperature. Of course, globe temperature includes exactly only air and radiant temperature thus as a criterion of human comfort the relationship on other factors must be taken into account, on air velocity and humidity, clothing, activity, adaptation and exposure time.

What is valid for the whole GT can be written approximately also for a part of it, for its segment. For GT of 15cm in diameter six segments have been proved quite satisfactory (originally 18 segments were tested). The surface temperature of each segment is called stereotemperature, i.e. the mean value of all six stereotemperatures equals

globe temperature.

For the scheme of instrument see Fig. 3 and Fig. 4 there is a photo. It is produced by SIPOCH Ltd. Prague. The company also developed electronics and technology of the instrument (dipl. Ing. L. Vajner).

Supposing a) the equality of heat transfer coefficients for irradiated and non-irradiated segment, b) the stereotemperature of non-irradiated segment equals globe temperature, the simple equation based on segments heat balance can be derived

$$t_{rA} - t_{rB} = (t_{stereo} - t_g) \left(1 + \frac{h_c}{h_r}\right)$$

$$t_{rA} - t_{rB} = (t_{stereo} - t_g) \left(1 + \frac{h_c}{h_r}\right)$$

where $t_{rA} - t_{rB}$ RTA [°C]

t_{stereo} stereotemperature, i.e. temperature of exposed segment [°C]

t_g globe temperature [°C]

h_c heat transfer coefficient by convection [$W^{-1}.m^2.K$]

h_r heat transfer coefficient by radiation [$W^{-1}.m^2.K$]

These equations cannot be applied in practice because the calculation of heat transfer coefficients is a difficult problem. Therefore the experimental estimation of equations is necessary.

Experimental estimation of the relationship between RTA and the difference stereotemperature minus globe temperature

The impact of vertical and horizontal surface has been tested in the climatic chamber (dimensions 3x2x2 m) (Fig. 5). Keeping globe temperature constant 24 °C the temperatures of the vertical surfaces was chosen 14, 19, 24, 29, 34 a 44 °C ,the temperatures of the horizontal surfaces 45, 53 a 58 °C (Tab. 2).

Tab. 2 Conditions in climatic chamber

VERTICAL RADIANT SURFACE							HORIZONTAL RADIANT SURFACE					
Exp.No.	t_g (°C)	t_{rA} (°C)	$\Delta t_{rA}-t_g$ (°C)	Exp.No.	t_g (°C)	t_{rA} (°C)	$\Delta t_{rA}-t_g$ (°C)	Exp.No.	t_g (°C)	t_{rA} (°C)	$\Delta t_{rA}-t_g$ (°C)	V
1	24	24	0	4	24	29	+5	7	24	45	21	1
2	24	14	-10	5	24	34	+10	8	24	53	29	1

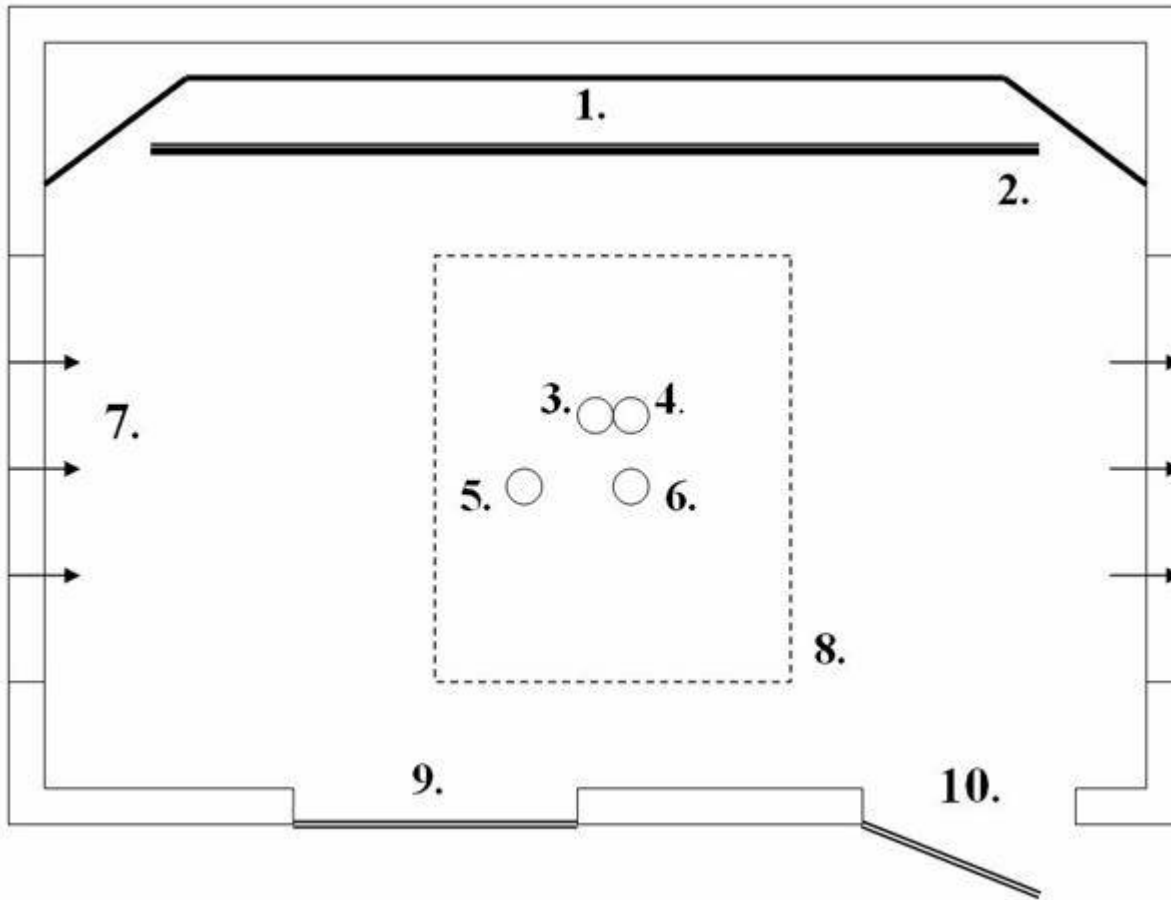


Figure 5. Measurements in climatic chamber, where 1. vertical warm radiant panel, 2. vertical cool radiant panel, 3. radiant temperature, 4. stereothermometer, 5. air velocity, 6. globe thermometer Vernon-Jokl, 7. direction of air flow, 8. ceiling radiant panel, 9. control room window, 10. entrance.

RTA, t_{rA} , t_{rB} , air flow velocities(chosen 0.25 m/s, 0.5 m/s a 1.0 m/s) air temperatures, relative air humidities were measured by Indoor Climate Analyzer Type 1213(Bruel and Kjaer) respecting EN ISO 7726.

The stereotemperatures t_{stereo} (the temperature of the exposed segment) and globe temperature were measured by stereothermometer.

The results are presented in Fig. 6 a 7.

The temperature t_{rA} (temperature of the irradiated plane side) against the stereotemperature (temperature of the irradiated segment) for three velocities (0.25 m/s, 0.5 m/s and 1.0 m/s) is presented in Fig. 6. Correlation coefficients are high ($R^2=0.9797$ up to 0.9908), thus the graph can be applied to practice for the estimation of t_{rA} on the basis of measured stereotemperature

$$t_{rA} = 3.4153 t_{stereo} - 57.004 \quad [^{\circ}\text{C}] \quad \text{for } v=0.25 \text{ m/s} \quad (3)$$

$$t_{rA} = 4.14 t_{stereo} - 74.971 \quad [^{\circ}\text{C}] \quad \text{for } v=0.5 \text{ m/s} \quad (4)$$

$$t_{rA} = 5.46 t_{stereo} - 108.33 \quad [^{\circ}\text{C}] \quad \text{for } v=1.0 \text{ m/s} \quad (5)$$

RTA ($=t_{rA} - t_{rB}$) depends on the difference stereotemperature minus globe temperature (t_{stereo} minus t_g), see Fig. 7. and following equations:

$$t_{rA} - t_{rB} = 3.6242(t_{stereo} - t_g) - 0.5098 \text{ [}^\circ\text{C]} \text{ for } v=0,25 \text{ m/s} \quad (6)$$

$$t_{rA} - t_{rB} = 4.3807(t_{stereo} - t_g) - 1.3907 \text{ [}^\circ\text{C]} \text{ for } v=0.5 \text{ m/s} \quad (7)$$

$$t_{rA} - t_{rB} = 5.1507(t_{stereo} - t_g) - 0.2010 \text{ [}^\circ\text{C]} \text{ for } v=1.0 \text{ m/s} \quad (8)$$

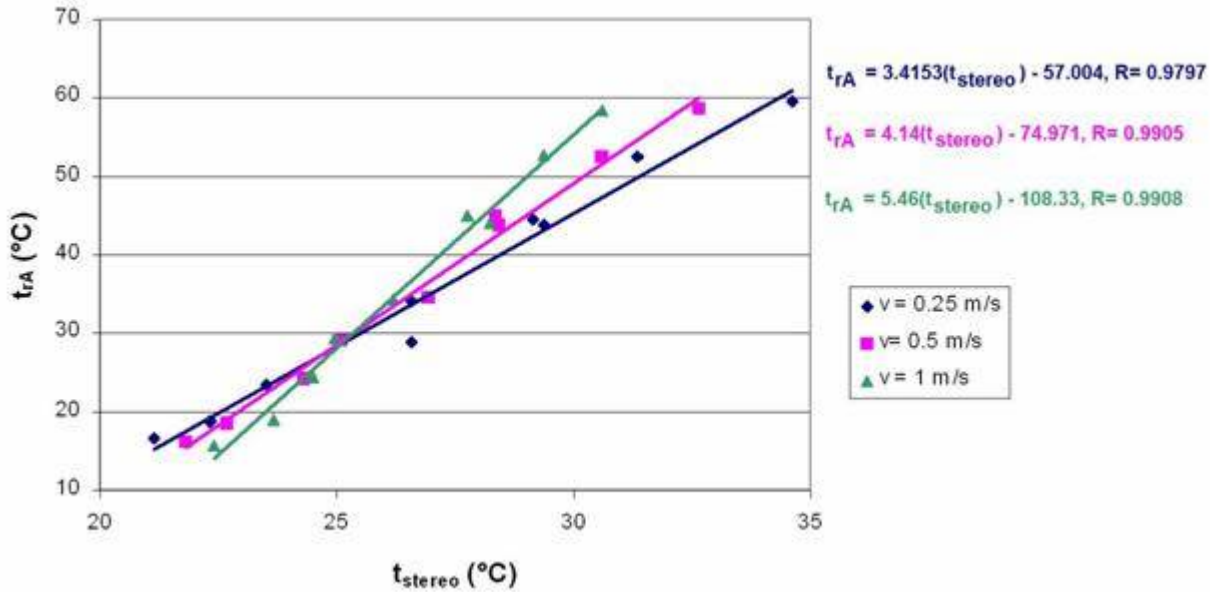


Figure 6. Relationship $t_{rA}=f(t_{stereo})$ for various v from experiments

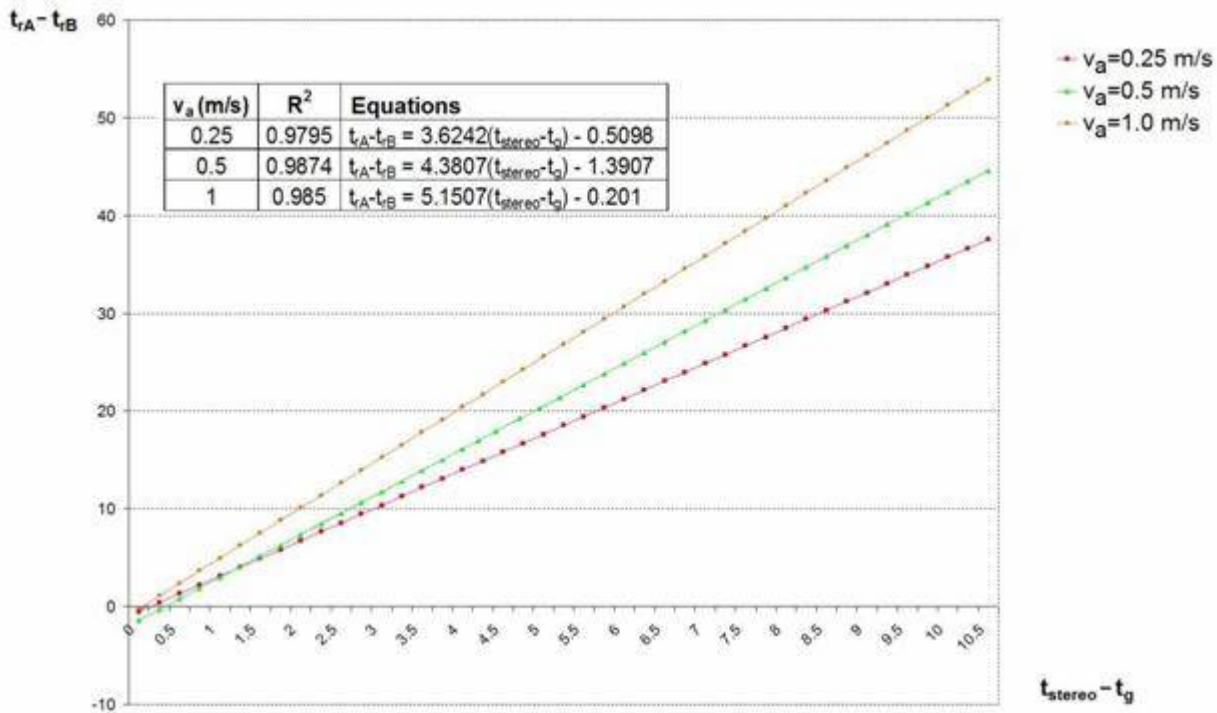


Figure 7. Relationship $RTA = t_{rA} - t_{rB} = f(t_{\text{stereo}} - t_g)$ from experiments.

Discussion

The estimation of RTA has been possible only by Indoor Climate Analyzer (Bruel and Kjaer) up to now. The instrument is highly sophisticated and thus expensive. A new instrument, globe stereothermometer, can be also used for this purpose being much more simple and thus cheaper. Electronics and technology of this instrument was also a problem; being solved enough is now produced professionally by SIPOCH Company.

Conclusion

The new instrument - globe stereothermometer - is a globe of 15cm in diameter divided into 6 segments; the segments temperature is called stereotemperature. Based on measurements in climatic chamber it has been proved that instrument allows estimation of RTA from the difference t_{stereo} minus t_g , see Fig.7 and equations (6),(7)and(8).

References

- EN ISO 7726. *Ergonomics of the thermal environment-Instruments for measurements of physical quantities*. 1998.
- EN ISO 7730. *Ergonomics of the thermal environment - Analytical determination and interpretation of thermal comfort using calculation of the PMV and PPD indices and local comfort criteria*. 2005.
- JIRÁK, Z.; JOKL, M. V., ŠEBASTA, D.; TOMÁŠKOVÁ, H., BERNATÍKOVÁ, Š.; MALÝ, S. 2007. Use of Globe Stereo Thermometer for Evaluation of Irregular Radiation Load. *Central European Journal of Public Health*, 2007, Supplement, vol. 15 (JHEMI vol. 51), p. S24.
- JOKL, M. V. 1966. The way of infrared heat load estimation over the human body surface. In Cech, Patent No. 117894, Prague.
- JOKL, M. V.; TŮMA, V. 1988. Directional globe thermometer. In Czech. Patent No.236203. Prague.
- JOKL, M. V. 1990. The stereothermometer: A new instrument for hygrothermal constituent nonuniformity evaluation. *ASHRAE Transactions* 96, 1990, No. 3435, p. 13-18.
- JOKL, M. V. 1991. Feuchtemessung nach "Kunstkopf" : prinzip. *Heizung-Luftung-Haustechnik*, 1991, vol. 42, no. 1, p. 27-32.
- JOKL, M. V. 1991. Stereoteploměr : nový přístroj pro hodnocení nerovnoměrnosti tepelně-vlhkostní konstituenty prostředí. *Československá hygiena*, 1991, vol. 36, no. 1, p. 14-23.
- JOKL, M. V. 2002. *Health Residential and Working Environment*. Prague : Czech Academia, 2002.
- JOKL, M. V.; VAJNER, L. 2003. Globe Thermometer : Useable Pattern No. 13547. Written down 1.8.2003. Owner VÚBP Prague.
- PETRÁŠ, D., KOUDELKOVÁ, D.; KABELE, K. 2004. *Hydronic and Electrical floor Heating*. Bratislava : Czech. Jaga,, 2004.

Autor článku:

[Prof. Ing. Miloslav Jokl, DrSc.](#)
[RNDr. Stanislav Malý, Ph.D. DBA](#)
[Prof. MUDr. Zdeněk Jirák, CSc.](#)
[Ing. Hana Tomášková, Ph.D.](#)
[Ing. Daniel Šebesta, Ph.D.](#)